

Owner's Manual

Wrist-type Fully Automatic Blood Pressure Monitor

Model BSP-22



Document No.:DBP-4004-021
Version: Z
Date of Issue: 2015.10

Contact Information

The lay operator or lay responsible or ganization should contact the manufacturer or the representative of manufacturer.
-for assistance,if needed,in setting up,using or maintaining the product,or
-to report unexpected operation or events.
Manufactured by Hangzhou Sejoy Electronics & Instruments Co., Ltd. Building 2, No. 202, Zhenzhong Road, West Lake Economy & Technology Zone, 310030 Hangzhou, China
Email: info@sejoy.com
Telephone: +86-571-81957767
Fax: +86-571-81957750

Contents

Safety Notice	02
Unit Illustration	06
Important Testing Guidelines	09
Quick Start	10
Unit Operation	12
Battery Installation	12
System Settings	13
Applying The Wrist Monitor	16
Testing	18
Power Off	23
Memory Check and Last 3 Tests Average	25
Memory Deletion	27
Low Battery Indicator	28
Troubleshooting	29
Blood Pressure Information	30
Blood Pressure Q&A	34
Maintenance	36
Specifications	40
Warranty	44
Electromagnetic Compatibility Information	45

1

Safety Notice

2

Thank you for purchasing the BSP-22 Blood Pressure Monitor. The unit has been constructed using reliable circuitry and durable materials. Used properly, this unit will provide years of satisfactory use.

Measure blood pressure (systolic and diastolic) and pulse rate of adults and adolescents age 12 through 21 years of age. All functions can be used safely and values can be read out in one LCD DISPLAY. Measurement position is on adult upper wrist only.

Blood pressure measurement determined with this device are equivalent to those obtained by a trained observer using the cuff/ stethoscope auscultation method, within the limits prescribed by the Recognized Consensus Standard(IEC 81060-2-30) for electronic sphygmomanometers.

Precautions to Ensure Safe, Reliable Operation

1. Do not drop the unit. Protect it from sudden jars or shocks.
2. Do not insert foreign objects into any openings.
3. Do not attempt to disassemble the unit.
4. Do not crush the pressure cuff.
5. If the unit has been stored at temperatures below 0 °C, leave it in a warm place for about 15 minutes before using it. Otherwise, the cuff may not inflate properly.
6. If the unit has been stored at temperatures above 40 °C,leave it in a cool place for about 15 minutes before using it. Otherwise, the cuff may not inflate properly.
7. Do not store the unit in direct sunlight, high humidity or dust.
8. To avoid any possibility of accidental strangulation, keep this unit away from children and do not drape tubing around your neck.
9. Ensure that children do not use the instrument unsupervised; some parts are small enough to be swallowed.
10. Some may get a skin irritation from the cuff taking frequent readings over the course of the day, but this irritation typically goes away on its own after the monitor is removed.

Safety Notice

3

Important Instructions Before Use

1. Do not confuse self-monitoring with self-diagnosis. Blood pressure measurements should only be interpreted by a health professional who is familiar with your medical history.
2. Contact your physician if test results regularly indicate abnormal readings.
3. If you are taking medication, consult with your physician to determine the most appropriate time to measure your blood pressure. NEVER change a prescribed medication without first consulting with your physician.
4. Individuals with serious circulation problems may experience discomfort. Consult your physician prior to use.
5. For persons with irregular or unstable circulation resulting from diabetes, liver disease, arteriosclerosis or other medical conditions, there may be variations in blood pressure values measured at the wrist versus at the upper arm. Monitoring the trends in your blood pressure taken at either the arm or the wrist is nevertheless useful and important.
6. People suffering from vascular constriction, liver disorders or diabetes, people with cardiac pacemakers or a weak pulse, and women who are pregnant should consult their physician before measuring their blood pressure themselves. Different values may be obtained due to their condition.
7. People suffering from arrhythmias such as atrial or ventricular premature beats or atrial fibrillation only use this blood pressure monitor in consultation with your doctor. In certain cases oscillometric measurement method can produce incorrect readings.
8. Too frequent measurements can cause injury to the patient due to blood flow interference.
9. The cuff should not be applied over a wound as this can cause further injury.


Safety Notice





4

10. DO NOT attach the cuff to a limb being used for IV infusions or any other intravascular access, therapy or an arterio-venous (A-V) shunt. The cuff inflation can temporarily block blood flow, potentially causing harm to the patient.
11. The cuff should not be placed on the arm on the side of a mastectomy. In the case of a double mastectomy use the side of the least dominant arm.
12. Pressurization of the cuff can temporarily cause loss of function of simultaneously used monitoring equipment on the same limb.
13. A compressed or kinked connection hose may cause continuous cuff pressure resulting in blood flow interference and potentially harmful injury to the patient.
14. Check that operation of the unit does not result in prolonged impairment of the circulation of the patient.
15. Product is designed for its intended use only. Do not misuse in anyway.
15. Product is designed for its intended use only. Do not misuse in any way.
16. Product is not intended for infants or individuals who cannot express their intentions.
17. Prolonged over-inflation of the bladder may cause ecchymoma of your arm.
18. Do not disassemble the unit or wrist cuff. Do not attempt to repair.
19. Use only the approved wrist cuff for this unit. Use of other wrist cuffs may result in incorrect measurement results.
20. The system might produce incorrect readings if stored or used outside the manufacturer's specified temperature and humidity ranges.

Unit Illustration

5


21. Do not use the device near strong electrical or electromagnetic fields generated by cell phones or other devices, they may cause incorrect readings and interference or become interference source to the device. Do not use the device during patient transport outside healthcare facility for interference source existing as well.
22. Do not mix new and old batteries simultaneously.
23. Replace batteries when Low Battery Indicator "⊗" appears on screen. Replace both batteries at the same time.
24. Do not mix battery types. Long-life alkaline batteries are recommended.
25. Remove batteries from device when not in operation for more than 3 months.
26. Do not insert the batteries with their polarities incorrectly aligned.
27. Dispose batteries properly; observe local laws and regulations.
28.  Advising operator that Instruction manual/ Booklet must be consulted

WARNING SIGNS AND SYMBOLS USED	
	Keep off Sunlight
	Type BF Equipment
	Instructions For Use MUST be Consulted
	Discard the used product to the recycling collection point according to local regulations

Unit Illustration

6


Monitor Unit

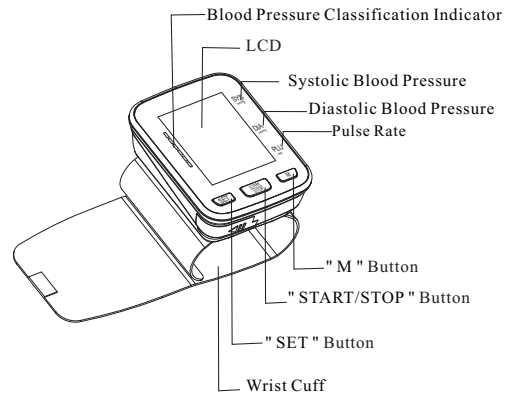

Unit Illustration

7


Display

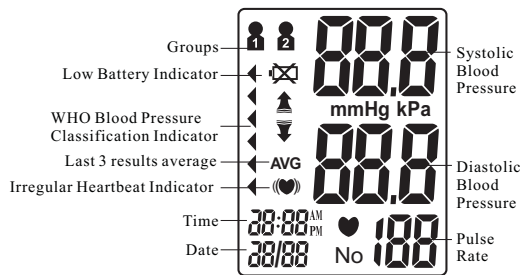

Unit Illustration

8

Contents

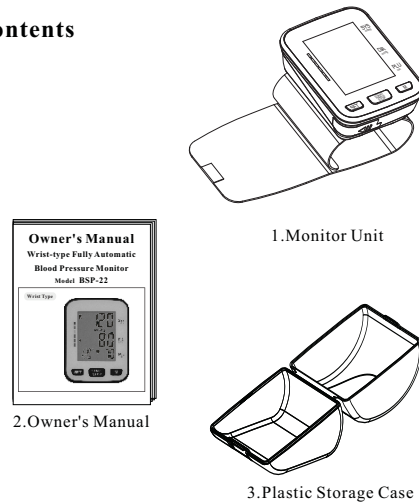

Important Testing Guidelines

9

1. Avoid eating, exercising, and bathing for 30 minutes prior to testing.
2. Sit in a calm environment for at least 5 minutes prior to testing.
3. Do not stand while testing. Sit in a relaxed position while keeping your wrist level with your heart.
4. Avoid speaking or moving body parts while testing.
5. While testing, avoid strong electromagnetic interference such as microwave ovens and cell phones.
6. Wait 3 minutes or longer before re-testing.
7. Try to measure your blood pressure at the same time each day for consistency.
8. Test comparisons should only be made when monitor is used on the same wrist, in the same position, and at the same time of day.
9. This blood pressure monitor is not recommended for people with severe arrhythmia.
10. Do not use this blood pressure monitor if the device is damaged.

Quick Start

10

1. Install batteries. (See Figure A)




Figure A

2. Remove clothing from the wrist area. (See Figure B)
3. Rest for several minutes prior to testing. Wrap cuff around left wrist. (See Figure C)




Figure B




Figure C

Quick Start

11

4. Sit in a comfortable position and place wrist level with heart.
(See Figure D)
5. Press "START/STOP" button to start testing. (See Figure E)



Figure D




Figure E

Unit Operation


12

Battery Installation


Slide battery cover off as indicated by arrow.

Install 2 new AAA alkaline batteries according to polarity.

Close battery cover.

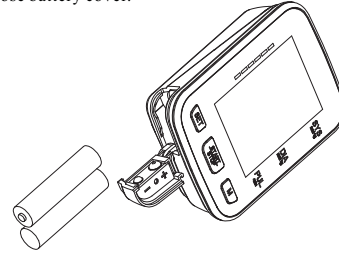

Note:

- 1) Replace batteries when Low Battery Indicator "  " appears on screen.
- 2) Batteries should be removed from device when not in operation for an extended period of time.

Unit Operation

13


System Settings

With power off, press "SET" button to actuate system setting. The Memory Group icon flashes.

1. Select memory Group

While in the System Setting mode you may accumulate test results into 2 different groups. This allows multiple users to save individual test results (up to 60 memories per group).

Press "M" button to choose a group setting. The test results will automatically store in each selected group.

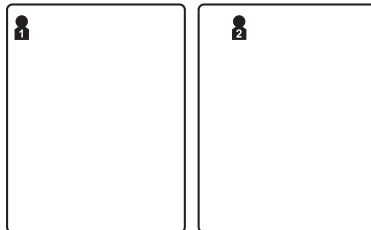

Unit Operation

14

2. Time/Date setting

Press "SET" button again to set the Time/Date mode. Set the year first by adjusting the "M" button. Press "SET" button again to confirm current month. Continue setting the day, hour and minute in the same way. Every time the "SET" button is pressed, it will lock in your selection and continue in succession (month, day, hour, minute)



Unit Operation


15

3. Time Format Setting.

Press "SET" button again to set the time format mode.

Set the time format by adjusting the "M" button.

EU means European Time US means U.S Time.

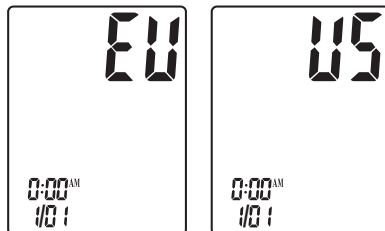

4. Save Settings

While in any setting mode, press "START/STOP" button to turn the unit off. All information will be saved.

Note: Unit will automatically save all information and shut off if left idle for 3 minutes.


Unit Operation

16

Applying The Wrist Monitor

Do not apply over clothing. If wearing a long sleeved shirt, be sure to roll sleeve back to forearm.


Apply monitor to wrist as illustrated. Tighten cuff firmly as not to wiggle.

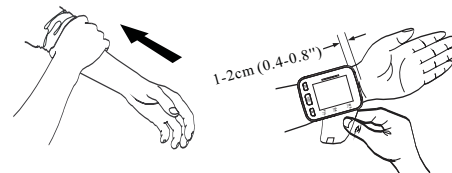

Unit Operation

17

Do not stand while testing. Sit in a comfortable position with back supported, feet flat on the floor with legs uncrossed. Place middle of the cuff at the level of the right atrium of the heart.




Unit Operation

18

Testing

1. Power On

Press and hold "START/STOP" button until a beep sounds. The LCD screen will appear for one second as unit performs a quick diagnosis. A long tone indicates device is ready for testing.




Note: Unit will not function if residual air from previous testing is present in cuff. The LCD will flash "↓" until pressure is stabilized.

Unit Operation

19

2. Pressurization

The unit will automatically inflate to the proper shelf and stop inflating. During this time, please keep quiet.



Note: Pressurization will gradually subside and ultimately stop when cuff is not properly applied to the wrist. If this occurs, press "START/STOP" button to turn the unit off.

Unit Operation

20

3. Testing

After cuff inflation, air will slowly subside as indicated by the corresponding cuff pressure value. A flashing "♥" will appear simultaneously on screen signaling heart beat detection.




Note: Remain relaxed during testing. Avoid speaking or moving body parts.

Unit Operation

21

4. Result Display

Three short beeps sound when testing is complete. The screen will display measurements for systolic and diastolic blood pressure. An indicator representing the current measurement will appear next to the corresponding WHO Classification.



Unit Operation

22

Note: Refer to Page 31~32 for detail WHO Blood Pressure Classification Information.

Irregular Heartbeat Indicator

If the monitor detects an irregular heart rhythm two or more times during the measuring process, the Irregular Heartbeat Symbol " (♥) " appears on screen along with measurement results. Irregular heartbeat rhythm is defined as rhythm that is either 25% slower or faster than the average rhythm detected while measuring systolic blood pressure and diastolic blood pressure. Consult your physician if the Irregular Heartbeat Symbol " (♥) " frequently appears with your test results.

Unit Operation

23

5. Deleting/Storing Test Results

User may delete their current test result due to unfavorable testing conditions or for any other reason. To delete the last test result, press the "SET" button after result is displayed. If result is not deleted, it will automatically store by date within the previously configured Memory Group.

Note: Be sure the appropriate Memory Group selection is made prior to testing.

If the number of tests surpasses the allotted 60 memories per group, the most recent tests will appear first, thus eliminating older readings.

Unit Operation

24

Power Off

The "START/STOP" button can be pressed to turn off the unit in any mode.

The unit can turn off the power itself about 3 minutes no operation in any mode.

Safety Precaution: If pressure in cuff becomes too extreme while testing, press the "START/STOP" button to turn power off.


The cuff pressure will rapidly dissipate once the unit is off.

Unit Operation

25

Memory Check and Last 3 Tests Average


With power off, press the "M" button to activate screen display. After the unit performs a self diagnosis, the screen will display the average test results from the last 3 readings of the last group used. The "AVG" symbol will appear along with the corresponding WHO Blood Pressure Indicator. To check the average results from other groups, select the desired group first prior to activating the "M" button in the off position (See "Select Memory Group" on page 13).



Unit Operation

26

Press the "M" button again, you may check past test results. Upon activating test results, you can press the "M" button to scroll through all test results stored in memory. The LCD will display the last memory as NO: 01 reading.

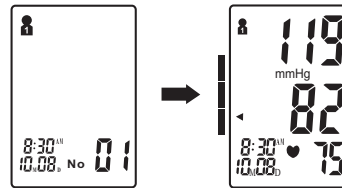


Note: Past test results will only be displayed from the most recently used memory group. To check past test results in other memory groups, you must first select the desired group and then turn monitor off. (See Select Memory Group on Page 13.)

Unit Operation

27

Memory Deletion

Memory for a selected group may be deleted while in Memory Check mode. Press and hold the "SET" button for approximately 3 seconds to delete all memory records from the selected group. The monitor will beep indicating successful deletion and then transfer into testing mode. To delete memories from other groups, please refer to "Select Memory Group" on page 10. Then press the "START/STOP" button to turn the unit off.




Note: Memory cannot be recovered once it has been deleted.

Unit Operation

28

Low Battery Indicator

4 short warning beeps sound when battery life is depleting and unable to inflate cuff for testing. The "X" symbol appears simultaneously for approximately 5 seconds prior to shutting down. Replace batteries at this time. No memory loss will occur throughout this process.




Unit Operation

29

Static Pressure Measurement

In the power down state, press and hold the "START/STOP" button, and then install the batteries. until the LCD screen is full, release the " START/STOP" button. When the LCD screen displays the double zero, the bloodpressure meter is in static state. Software version is displayed at the heart rate .



Note: Only Service personnel permitted to access to this mode, the mode unavailable in normal use.

Unit Operation

30

Troubleshooting

Problem	Possible Cause	Solution
Blood pressure results are not within typical range	Cuff is too tight or not properly positioned on the wrist	Firmly reposition cuff on wrist making sure no wiggle is present. (See Page 15)
	Inaccurate test results due to body movement or monitor movement	Sit in a relaxed position placing wrist level with heart. Avoid speaking or moving body parts while testing. (See Page 8)
" Err " displayed	Cuff fails to inflate properly	Make sure hose is properly fastened to cuff and monitor unit
	Improper operation	Read user manual carefully and re-test properly.
	Pressurization is over cuff rated pressure 300mmHg	Read user manual carefully and re-test properly.

Blood Pressure Information


31

Blood Pressure

Blood pressure is the force of blood pushing against the walls of arteries. It is typically measured in millimeters of mercury (mmHg.) Systolic blood pressure is the maximum force exerted against blood vessel walls each time the heart beats. Diastolic blood pressure is the force exerted on blood vessels when the heart is resting between beats.

An individual's blood pressure frequently changes throughout the course of a day. Excitement and tension can cause blood pressure to rise, while drinking alcohol and bathing can lower blood pressure. Certain hormones like adrenaline (which your body releases under stress) can cause blood vessels to constrict, leading to a rise in blood pressure.

If these measuring numbers become too high, it means the heart is working harder than it should.

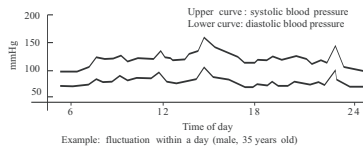


Blood Pressure Information


32

WHO Blood Pressure Classification Indicator

The BSP-22 is equipped with a classification indicator based on established guidelines from the World Health Organization. The chart below (color coded on monitor unit) indicates test results.



Mild Hypertension




■: Blood Pressure Classification Indicator

Blood Pressure Information

33

Health Reminder

Hypertension is a dangerous disease that can affect the quality of life. It can lead to a lot of problems including heart failure, kidney failure, and cerebral hemorrhaging. By maintaining a healthy lifestyle and visiting your physician on a regular basis, hypertension and relative diseases are much easier to control when diagnosed in the early stages.

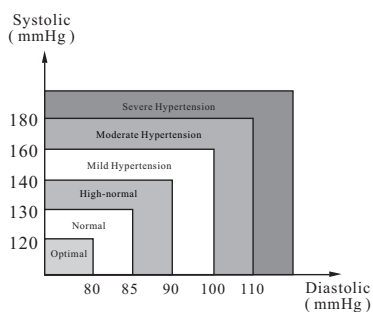

Blood Pressure Information

34

Note: Do not be alarmed if an abnormal reading occurs. A better indication of an individual's blood pressure occurs after 2-3 readings are taken at the same time each day over an extended period of time. Consult your physician if test results remain abnormal.

Blood Pressure Q&A

35

- Q:** What is the difference between measuring blood pressure at home or at a professional healthcare clinic?
- A:** Blood pressure readings taken at home are now seen to give a more accurate account as they better reflect your daily life. Readings can be elevated when taken in a clinical or medical environment. This is known as White Coat Hypertension and may be caused by feeling anxious or nervous.

Note: Abnormal test results may be caused by:

1. Improper cuff placement
Make sure cuff is snug-not too tight or too loose.
2. Improper body position
Make sure to keep your body in an upright position.
3. Feeling anxious or nervous
Take 2-3 deep breaths, wait a few minutes and resume testing.

Blood Pressure Q&A


36

- Q:** What causes different readings?
- A:** Blood pressure varies throughout the course of a day. Many factors including diet, stress, cuff placement, etc. may affect an individual's blood pressure.
- Q:** Should I apply the cuff to the left or right wrist? What is the difference?
- A:** Either wrist can be used when testing, however, when comparing results, the same wrist should be used. Testing on your left wrist may provide more accurate results as it is located closer to your heart.
- Q:** What is the best time of day for testing?
- A:** Morning time or any time you feel relaxed and stress free.

Maintenance

37

1. Avoid dropping, slamming, or throwing the unit.




2. Avoid extreme temperatures. Do not use outdoors.




Maintenance

38

3. When cleaning the unit, use a soft fabric and lightly wipe with mild detergent. Use a damp cloth to remove dirt and excess detergent.




4. Cuff Cleaning: Do not soak cuff in water! Apply a small amount of rubbing alcohol to a soft cloth to clean cuff's surface. Use a damp cloth (water-based) to wipe clean. Allow cuff to dry naturally at room temperature. The cuff must be cleaned and disinfected before use between different users.




Maintenance

39

5. Do not use petrol, thinners or similar solvents.




6. Remove batteries when not in operation for an extended period of time.



Maintenance

40

7. Do not disassemble product.



8. It is recommended the performance should be checked every 2 years.
9. Expected service life: Approximately three years at 10 tests per day.
10. No service and maintenance while it is in use and maintenance only be performed by service personnel. Service and maintenance require parts, repair, technical support will be provided.


Specifications

41

Product Description	Wrist-Type Fully Automatic Digital Blood Pressure Monitor	
Model	BSP-22	
Display	LCD Digital Display Size:49mm×38mm	
Measurement Method	Oscillometric Method	
Measurement Range	Systolic Pressure	60mmHg~280mmHg
	Diastolic Pressure	30mmHg~200mmHg
	Pressure	0mmHg~300mmHg
	Pressure	±3mmHg or ±2% of the reading above 200 mmHg
	Pulse	30 ~ 180 Beats/Minute
	Pulse	±5%
Pressurization	Automatic Pressurization	
Memory	120 Memories in Tow Groups with Date and Time	
Function	Irregular Heartbeat Detection	
	WHO Classification Indicator	
	Last 3 Results Average	
	Low Battery Detection	
	Automatic Power-Off	

Specifications

42

Function	Backlight	
Power Source	2 Alkaline Batteries Size AAA	
Battery Life	Approximately 2 months at 3 tests per day	
Unit Weight	Approx. 115g (4.06oz.) (Excluding Battery)	
Unit Dimensions	Approx. 84 x 64 x 29mm (3.31" x 2.52" x 1.14")(L x W x H)	
Cuff Circumference	13.5-21.5 cm	
Operating Environment	Temperature	10°C ~ 40°C (50□~104□)
	Humidity	15%~93%RH
	Pressure	700hPa~1060hPa
Storage Environment	Temperature	-25°C~70°C (-13□~158□)
	Humidity	≤93% RH
Ingress Protection Rating:	IP 22	
Classification	Internal Powered Equipment Type BF 	

Specifications are subject to change without notice.

Specifications

43

- IEC 80601-2-30, medical electrical equipment - part 2-30: particular requirements for the basic safety and essential performance of automated noninvasive sphygmomanometers. (Cardiovascular)
- ANSI/AAMI ISO 81060-2, non-invasive sphygmomanometers - part 2: clinical validation of automated measurement type. (Cardiovascular)
- AAMI / ANSI ES60601-1:2005/(R)2012 and C1:2009/(R)2012 and, a2:2010/(r)2012 (consolidated text) medical electrical equipment -- part 1: general requirements for basic safety and essential performance
- AAMI/ANSI/IEC 60601-1-2, Medical Electrical Equipment -- Part 1-2: General Requirements For Basic Safety And Essential Performance -- Collateral Standard: Electromagnetic Disturbances -- Requirements And Tests (General II (ES/EMC)).
- IEC 60601-1-11, medical electrical equipment - part 1-11: general requirements for basic safety and essential performance - collateral standard: requirements for medical electrical equipment and medical electrical systems used in the home healthcare environment.

Specifications

44

Correct Disposal of This Product
(Waste Electrical & Electronic Equipment)



This marking shown on the product indicates that it should not be disposed with other household waste at the end of its life. To prevent potential harm to the environment or to human health, please separate this product from other types of wastes and recycle it responsibly. When disposing this type of product, contact the retailer where product was purchased or contact your local government office for details regarding how this item can be disposed in an environmentally safe recycling center. Business users should contact their supplier and check the terms and conditions of the purchasing agreement. This product should not be mixed with other commercial wastes for disposal. This product is free of hazardous materials.

Warranty

45

The Blood Pressure Monitor is guaranteed for 2-year from the date of purchase. If the Blood Pressure Monitor does not function properly due to defective components or poor workmanship, we will repair or replace it freely. The warranty does not cover damages to your Blood Pressure Monitor due to improper handling. Please contact local retailer for details.

Electromagnetic Compatibility Information

46

The device satisfies the EMC requirements of the international standard IEC 60601-1-2. The requirements are satisfied under the conditions described in the table below. The device is an electrical medical product and is subject to special precautionary measures with regard to EMC which must be published in the instructions for use. Portable and mobile HF communications equipment can affect the device. Use of the unit in conjunction with non-approved accessories can affect the device negatively and alter the electromagnetic compatibility. The device should not be used directly adjacent to or between other electrical equipment.

Table 1

Guidance and declaration of manufacturer-electromagnetic emissions		
The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment -guidance
Radiated emission CISPR 11	Group 1, ClassB	The device uses RF energy only for its internal function. Therefore, its emissions are very low and are not likely to cause any interference in nearby electronic equipment.
Conducted emission CISPR 11	N/A	
Harmonic emissions IEC 61000-3-2	N/A	
Voltage fluctuations/ Flicker emissions IEC 61000-3-3	N/A	

Table 2

Guidance and declaration of manufacturer-electromagnetic immunity			
The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.			
IMMUNITY test	IEC 60601 test level	Compliance level	Electromagnetic environment -guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 8 kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV air	± 8 kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrostatic transient/burst IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input/output lines	N/A	
Surge IEC 61000-4-5	± 1 kV differential mode ± 2 kV common mode	N/A	
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5% UT (>95% dip in UT) for 0.5 cycle 40% UT (60% dip in UT) for 5 cycle 70% UT (30% dip in UT) for 25 cycle <5% UT (>95% dip in UT) for 5 secretary	N/A	
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m; 50Hz or 60Hz	30 A/m; 50Hz or 60Hz	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Table 3


Guidance and declaration of manufacturer-electromagnetic immunity			
The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.			
IMMUNITY test	IEC 60601 test level	Compliance level	Electromagnetic environment -guidance
Conducted RF IEC 61000-4-6	3V for 0.15-80 MHz; 6V in ISM and amateur radio bands between 0.15-80MHz	N/A	Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.
Radiated RF IEC 61000-4-3	385MHz, 27V/m	385MHz, 27V/m	Recommended separation distance $d = \left[\frac{3.5}{E_1} \right] \sqrt{P}$ 80 MHz to 800 MHz $d = \left[\frac{7}{E_1} \right] \sqrt{P}$ 800 MHz to 2.7 Ghz where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range. Interference may occur in the vicinity of equipment marked with the following symbol: 
	450MHz, 28V/m	450MHz, 28V/m	
	710MHz, 745 MHz, 780MHz 9V/m	710MHz, 745 MHz, 780MHz 9V/m	
	810MHz, 870 MHz, 930MHz 28V/m	810MHz, 870 MHz, 930MHz 28V/m	
	1720MHz, 1845 MHz, 1970MHz 28V/m	1720MHz, 1845 MHz, 1970MHz 28V/m	
2450MHz, 28V/m	2450MHz, 28V/m		
5240MHz, 5500 MHz, 5785MHz 9V/m	5240MHz, 5500 MHz, 5785MHz 9V/m		

Table 4

Recommended separation distances between portable and mobile RF communications equipment and the device		
The device is intended for use in an electromagnetic environment in which radiated therefore disturbances are controlled. The customer or the user of the device can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the device as recommended below, according to the maximum output power of the communications equipment.		
Rated maximum output power of transmitter	Separation distance according to frequency of transmitter	
W	80 MHz to 800 MHz $d = \left[\frac{3.5}{E_1} \right] \sqrt{P}$	800 MHz to 2.7 GHz $d = \left[\frac{7}{E_1} \right] \sqrt{P}$
0.01	0.12	0.23
0.1	0.38	0.73
1	1.2	2.3
10	3.8	7.3
100	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.